



HAL
open science

Non-intrusive pipe internal pressure measurement

Laurent Maurin, Nicolas Roussel, Guillaume Laffont

► **To cite this version:**

Laurent Maurin, Nicolas Roussel, Guillaume Laffont. Non-intrusive pipe internal pressure measurement. NURETH19 - 19th International Topical Meeting on Nuclear Reactor Thermal Hydraulics, Mar 2022, Bruxelles, Belgium. cea-03687703

HAL Id: cea-03687703

<https://cea.hal.science/cea-03687703v1>

Submitted on 3 Jun 2022

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



FROM RESEARCH TO INDUSTRY

Non-intrusive pipe internal pressure measurement

15:20-15:50, the 4th of March, 2022 – NURETH19 Workshop – Fiber-optic sensors for thermal hydraulic measurements

L. Maurin, N. Roussel & G. Laffont
Université Paris-Saclay, CEA, List, F-91120, Palaiseau, France



CEA - www.cea.fr

6 – 11 MARCH 2022, NURETH19, BRUSSELS, BELGIUM
19th International Topical Meeting on Nuclear Reactor Thermal Hydraulics



EUROPEAN NUCLEAR SOCIETY



FROM RESEARCH TO INDUSTRY

Non-intrusive pipe internal pressure measurement

15:20-15:50, the 4th of March, 2022 – NURETH19 Workshop – Fiber-optic sensors for thermal hydraulic measurements

L. Maurin, N. Roussel & G. Laffont
Université Paris-Saclay, CEA, List, F-91120, Palaiseau, France



CEA - www.cea.fr

6 – 11 MARCH 2022, NURETH19, BRUSSELS, BELGIUM
19th International Topical Meeting on Nuclear Reactor Thermal Hydraulics



EUROPEAN NUCLEAR SOCIETY



► Global context

- Why a non-intrusive pressure measurement ?

► Non-intrusive pressure measurement and temperature compensation background

- Non-intrusive pressure measurement – Background
- Temperature cross-sensitivity compensation based on the same proof body – Background

► Non-intrusive pressure measurement – Underlying principle and core theory

- Underlying principle leading to temperature cross-sensitivity compensation
- The infinitely long and straight pipe under hydrostatic pressure
- The FBG transducer – Some orders of magnitude
- Non-intrusive pressure ΔP_{int} measurement with direction-sensitive strain transducers
- Additional effects mitigation & application to other measurement techniques

► Experimental validations – From simple to more severe conditions

- I – Mechanically isolated pipe section
- II – Air pressure loop
- III – Water pressure loop (NPP primary coolant circuit)
 - Hot-air gun experiment to estimate the non-intrusive pressure measurement robustness
 - No fluid flow, no temperature change
 - No fluid flow, but temperature changes due to heat conduction
 - Fluid flow with massive fluid flow change (from 14 m³/h to zero) & temperature changes

► Conclusion

► Acknowledgements

► Additional information – Data availability



FROM RESEARCH TO INDUSTRY

Global context

15:20-15:50, the 4th of March, 2022 – NURETH19 Workshop – Fiber-optic sensors for thermal hydraulic measurements



CEA - www.cea.fr

6 – 11 MARCH 2022, NURETH19, BRUSSELS, BELGIUM
19th International Topical Meeting on Nuclear Reactor Thermal Hydraulics



EUROPEAN NUCLEAR SOCIETY



Why a non-intrusive pressure measurement ?

▶ No more pipe structural health damage due to sensor installation

- Does not require a hole per sensor
 - Measurement provided from pipe external surface, or even remotely
- Sensors can be installed and removed on demand, without any downtime, nor regualification

▶ No more contact with the fluid to monitor

- The pipe acts like the membrane of the traditional, but intrusive, sensor
 - But any undesired mechanical action on the pipe may introduce a measurement bias
 - Mitigation solution to be implemented to compensate for the effects of pure bending



e.g.: pressure equipment directive [97/23/EC](#) from EU



▶ A crucial measurement for the oil & gas industry

- First to prevent **hydrate-plugs** formation under specific **{P, T}** conditions (offshore)
- Second to **reduce the risk of pipe failure**, and subsequent environmental consequences

▶ Non-intrusive pressure sensors development mainly driven by the oil & gas industry

- Previous attempts mainly based on **ring sensors** (unsteady pressure), **surface strain measurements** or **acoustic waves**
 - Still suffer from **shortcomings**, with in general **poor temperature cross-sensitivity compensation**
- Only one solution (Ekechukwu, 2021) based on both **DAS** and **Raman DTS** led to **satisfactory** results

▶ New solution applicable to any fluid transportation if pipe cross-section is circular

- **Temperature cross-sensitivity** on pressure measurement **intrinsically compensated** / cancelled



FROM RESEARCH TO INDUSTRY

Non-intrusive pressure measurement and temperature compensation background

15:20-15:50, the 4th of March, 2022 – NURETH19 Workshop – Fiber-optic sensors for thermal hydraulic measurements



CEA - www.cea.fr


6 – 11 MARCH 2022, NURETH19, BRUSSELS, BELGIUM
19th International Topical Meeting on Nuclear Reactor Thermal Hydraulics



EUROPEAN NUCLEAR SOCIETY




Non-intrusive pressure measurement – Background

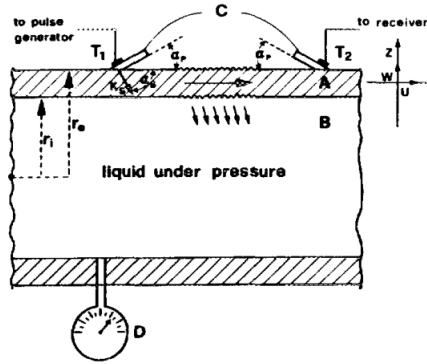


Diodati, 1986, **ultrasonics**
acoustic signal amplitude

→ dependency on fluid compressibility

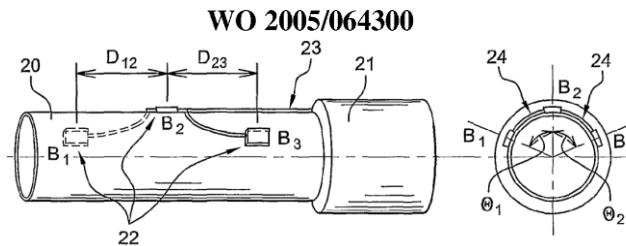


Magne *et al*, 2005, **FBG** strain rosette
surface strain

→ temperature compensation issue
→ thin-shell theory approximation

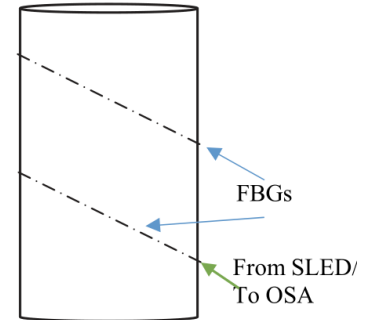


Meiring *et al*, 2016, **FBG**
placed helically around the pipe
surface strain

→ temperature compensation issue

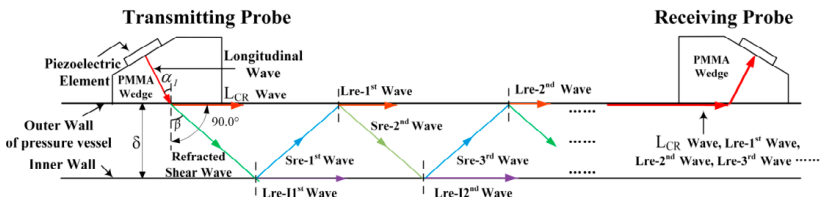


Zhou *et al*, 2016, **ultrasonics**
propagation time of multiple longitudinal waves

→ temperature dependency requiring calibration
→ thin-shell theory approximation

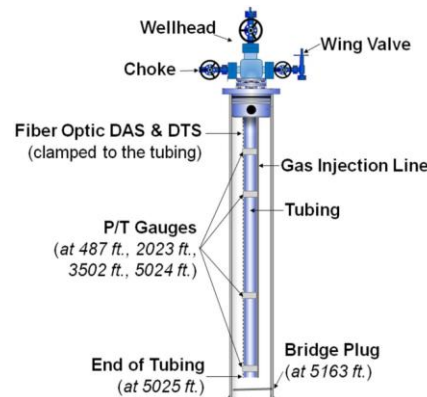





Ekechukwu *et al*, 2021, **DAS & Raman DTS**

low-frequency DAS components
→ questionable if the fluid does not flow

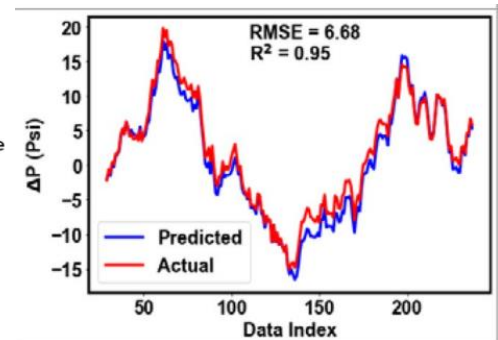




Temperature cross-sensitivity compensation based on the same proof body – Background

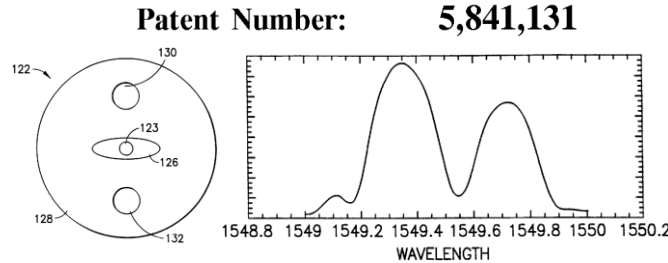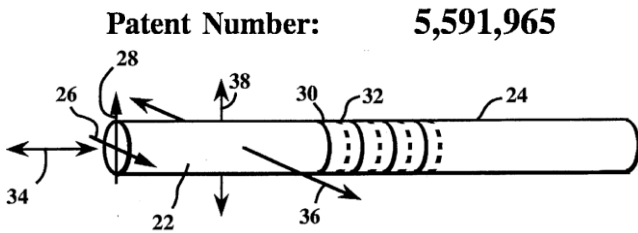

Udd, **1995**, **overlaid FBGs** at different wavelengths in **birefringent optical fiber**

Schroeder *et al*, **1997** (Schlumberger™) **FBG in birefringent optical fiber**

Chen *et al*, **2003**, **Hi-Bi FBG**

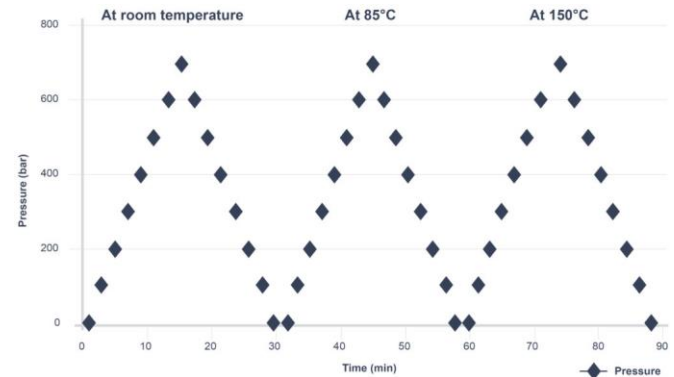

FBGS™ pressure sensor based on **Hi-Bi FBG**
<https://fbgs.com/solutions/pressure-sensing/>



Schlumberger™ **quartz** pressure sensor – Donzier *et al*, **2000**
 from “Techniques de l’Ingénieur”, vol. E 3 093
 (“Capteurs microélectroniques”)
 Pressure stability better than 0.01% Full Scale / Year



FROM RESEARCH TO INDUSTRY

Non-intrusive pressure measurement Underlying principle and core theory

15:20-15:50, the 4th of March, 2022 – NURETH19 Workshop – Fiber-optic sensors for thermal hydraulic measurements



CEA - www.cea.fr

6 – 11 MARCH 2022, NURETH19, BRUSSELS, BELGIUM
19th International Topical Meeting on Nuclear Reactor Thermal Hydraulics



EUROPEAN NUCLEAR SOCIETY



Underlying principle leading to temperature cross-sensitivity compensation

► Pipe behaviour under pressure well-known for decades – Formal models available

- **Materials' strength** recipes (Roark 1938) → *averaged* values over pipe sections, thin vs. thick models
- **Continuum mechanics** in the elastic range (Love 1927, Timoshenko 1934) → full & accurate solutions derived from Airy's potential – **Temperature dependency to be taken into account**


► Exhibits different hoop vs. longitudinal stress sensitivities under hydrostatic pressure

- Balance of pipe wall internal forces vs. forces resulting from internal pressure P_{int} (*closed pipe hypothesis*)

hoop: $2\sigma_{\theta\theta} \cdot e \cdot b \simeq P_{int} \cdot 2R \cdot b$ (*cylindrical cross-section balance*)
longitudinal: $\sigma_{zz} \cdot e \cdot 2\pi R \simeq P_{int} \cdot \pi R^2$ (*circular cross-section balance*)

($\sigma_{\theta\theta}$ and σ_{zz} are resp. the hoop & longitudinal cross-sectional average stresses)

$$P_{int} \simeq \frac{2\sigma_{\theta\theta} \cdot e \cdot b}{2R \cdot b} \simeq \frac{\sigma_{zz} \cdot e \cdot 2\pi R}{\pi R^2} \Rightarrow \boxed{\sigma_{\theta\theta} \simeq 2\sigma_{zz}} \quad (\text{thin-shell approximation})$$

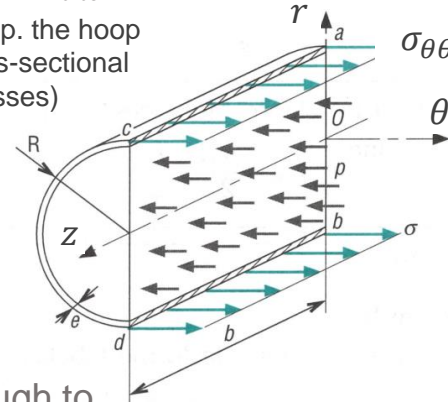

modified from Fanchon,
"Guide de mécanique", 1998



**temperature
compensation
paradigm different
from conventional
solutions**

⇒ In the elastic range, leads roughly to the same ratio between the *average* hoop $\varepsilon_{\theta\theta}$ and the longitudinal ε_{zz} mechanical strains, **BUT ...**

- ⇒ **Poisson's** transverse effect & **pipe thickness** do interfere significantly
- ⇒ **Thin-shell** model from material's strength approximation is not accurate enough to properly describe strains distribution within the pipe wall and on its surfaces

⇒ Provides a clue for intrinsic temperature cross-sensitivity compensation with orientation-sensitive strain transducers by simple subtraction of 2 raw measurements

- Requires a complete thermomechanical & accurate model
 - Expected better efficiency than the sole Poisson's transverse effect (Maurin *et al*, 2007)
- ⇒ **FBG transducers are good candidates for such implementation**



The infinitely long and straight pipe under hydrostatic pressure

► Elastic strains hypothesis

- Hooke's law: $[\sigma] = 2\mu[\varepsilon]_{mec} + \lambda \text{Tr}([\varepsilon]_{mec}) [I]$
- *Linearized* Green-Lagrange strain tensor $[\varepsilon]$ approximation:

$$\varepsilon_{ij} = \frac{1}{2} \left(\frac{\partial u_i}{\partial x_j} + \frac{\partial u_j}{\partial x_i} + \sum_{k=1}^3 \frac{\partial u_k}{\partial x_i} \frac{\partial u_k}{\partial x_j} \right)$$

► Problem formulated in terms of displacements

- $\vec{u} = \vec{u}_\sigma + \vec{u}_T$: total displacement \vec{u} (sum of mechanical \vec{u}_σ and thermal \vec{u}_T displacements)
- **Homogeneous temperature** in the pipe wall & **no shear stress** hypotheses
→ the temperature does not generate any additional mechanical strain

► Fundamental equation of dynamics for deformable bodies


$$\text{div} [\sigma] + \rho(\vec{f} - \vec{\gamma}) = \vec{0} \Rightarrow \text{div} [\sigma] \simeq \vec{0} \quad (\text{static conditions})$$

set of partial differential equations

formal solution valid *anywhere* in the pipe wall & pipe surfaces

displacement	$\vec{u} = f(K_1, L_1, L_2)$
strain tensor	$[\varepsilon] = g(K_1, L_1, L_2)$
stress tensor	$[\sigma] = h(K_1, L_1, L_2)$

- linear relationship with hydrostatic pressures
- quadratic relationship with temperature

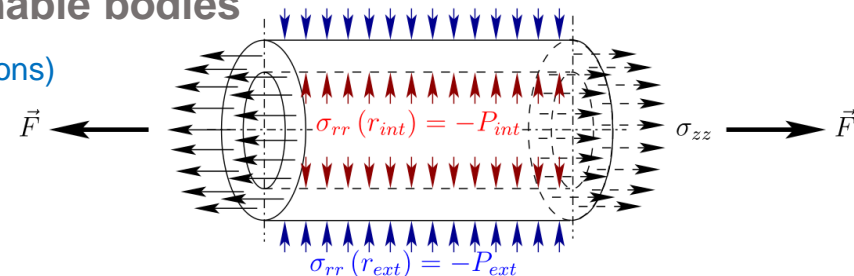

boundary conditions applied on the **straight pipe** section

- K_1, L_1, L_2 are integration parameters depending on:
- pipe thermomechanical properties,
 - pipe inner r_{0_int} & outer r_{0_ext} radiuses,
 - longitudinal pulling force \vec{F} ,
 - inner P_{int} & outer P_{ext} hydrostatic pressures,
 - surface temperature T .



The FBG transducer – Some orders of magnitude

► Temperature & strain measurements with the FBG transducer

$$\lambda_B = 2n_{eff}\Lambda \Rightarrow \frac{d\lambda_B}{\lambda_B} = (\kappa_T + \kappa_\varepsilon \cdot \Delta\alpha) \cdot dT + \kappa_\varepsilon \cdot d\varepsilon_{mec}$$

temperature dependency

mechanical strain dependency

- $\kappa_\varepsilon \cdot \Delta\alpha$: additional temperature sensitivity when attached to pipe surface

- Detached from the structure: $\Delta\lambda_B = 1 \text{ pm} \leftrightarrow 0.1^\circ\text{C} \leftrightarrow 1 \mu\text{m/m}$

- **Once attached to pipe surface:** $\Delta\lambda_B = 1 \text{ pm} \leftrightarrow 0.04^\circ\text{C} \leftrightarrow 1 \mu\text{m/m}$

- Typically **2.3 times more sensitive** to temperature

- Typical mechanical strain amplitude of a **Ø 4" NPS Sch. 160 metallic pipe** under hydrostatic pressure

- $\Delta P_{int} = 1 \text{ bar} \Rightarrow \Delta\varepsilon_{mec} \simeq 1 \mu\text{m/m} \Rightarrow \delta P_{int} = 1 \text{ bar resolution} \leftrightarrow 0.04^\circ\text{C max temperature discrepancy}$



⇒ **Temperature cross-sensitivity compensation is critical to reach $\delta P_{int} = 1 \text{ bar}$ resolution** (typical performance target)

► FBG temperature is mainly weighted by the pipe thermal effusivity



- Temperature discrepancy between 2 transducers attached to the pipe surface **remains very small**
- The **subtraction** between two raw measurements can therefore be assimilated to a **purely mechanical information, in direct relationship with the internal pressure in the elastic range**
 - λ_1 and λ_2 are the Bragg wavelengths of the FBG transducers attached to the pipe external surface

$$\Delta P_{int} \simeq f_{\Delta\varepsilon} (\Delta\lambda_1 - \Delta\lambda_2) \quad f_{\Delta\varepsilon}: \text{linear function}$$

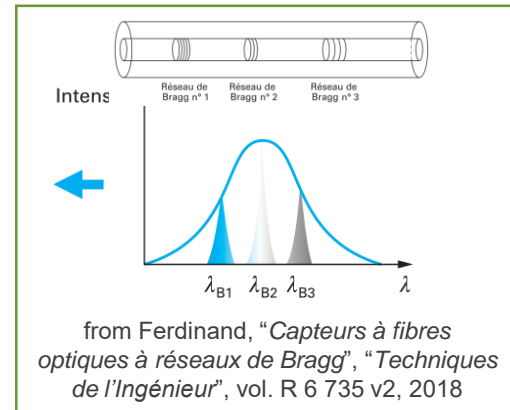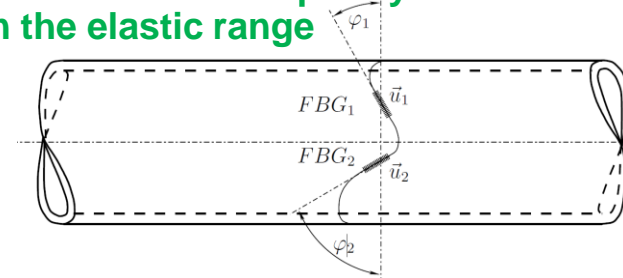

(@ 1550 nm)



Non-intrusive pressure ΔP_{int} measurement with direction-sensitive strain transducers

► Non-intrusive pressure measurement on a **straight** and **closed** pipe section

- Internal pressure ΔP_{int} and surface temperature ΔT variations are two independent information
 - Temperature variation ΔT also based on pipe mechanical properties (Young's modulus E & Poisson's ratio ν)
 - **Time delayed information** (due to heat diffusion) to be considered with limited confidence


$$\left\{ \begin{array}{l} \Delta P_{int} = \Delta P_{ext} + \frac{r_{0_{ext}}^2 E (\Delta \Psi_1 - \Delta \Psi_2)}{\kappa_\varepsilon (1 + \nu) [\cos^2(\varphi_1) - \cos^2(\varphi_2)]} \left(\frac{1}{r_{0_{int}}^2} - \frac{1}{r_{0_{ext}}^2} \right) + \frac{\delta F}{\pi r_{0_{int}}^2} \\ \Delta T = \frac{1}{\kappa_T} \left[\frac{1 - 2\nu}{1 + \nu} \frac{\Delta \Psi_1 - \Delta \Psi_2}{\cos^2(\varphi_2) - \cos^2(\varphi_1)} + \frac{\Delta \Psi_1 \cos^2(\varphi_2) - \Delta \Psi_2 \cos^2(\varphi_1)}{\cos^2(\varphi_2) - \cos^2(\varphi_1)} \right. \\ \left. + \frac{\kappa_\varepsilon (1 - 2\nu)}{E} \Delta P_{ext} - \frac{1}{\pi E} \frac{2\kappa_\varepsilon (1 - \nu)}{r_{0_{ext}}^2 - r_{0_{int}}^2} \delta F \right] \end{array} \right.$$

$\Delta \Psi$ the transducer true relative variation measurement

$$\Delta \Psi = \ln \left(1 + \frac{\Delta \lambda_B}{\lambda_B} \right) \underset{0}{\approx} \frac{\Delta \lambda_B}{\lambda_B}$$

δF is the unexplained residual longitudinal force


$$|\varphi_1| \neq |\varphi_2| \pmod{\pi}$$

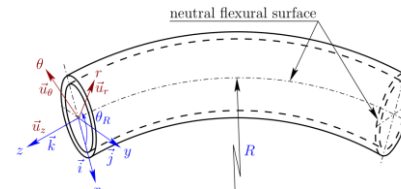

► Bending mitigation by simple averaging

- Requires $N \geq 2$ sensors evenly distributed in ring position around the pipe

$$\left\{ \begin{array}{l} \Delta P_{int} = \Delta P_{ext} + \frac{r_{0_{ext}}^2 E \left(\frac{1}{N} \sum_{k=1}^{k=N} (\Delta \Psi_{1k} - \Delta \Psi_{2k}) \right)}{\kappa_\varepsilon (1 + \nu) [\cos^2(\varphi_1) - \cos^2(\varphi_2)]} \left(\frac{1}{r_{0_{int}}^2} - \frac{1}{r_{0_{ext}}^2} \right) + \frac{\delta F}{\pi r_{0_{int}}^2} \\ \Delta T = \frac{1}{\kappa_T} \left[\frac{1 - 2\nu}{1 + \nu} \frac{\frac{1}{N} \sum_{k=1}^{k=N} (\Delta \Psi_{1k} - \Delta \Psi_{2k})}{\cos^2(\varphi_2) - \cos^2(\varphi_1)} + \frac{\frac{1}{N} \sum_{k=1}^{k=N} [\Delta \Psi_{1k} \cos^2(\varphi_2) - \Delta \Psi_{2k} \cos^2(\varphi_1)]}{\cos^2(\varphi_2) - \cos^2(\varphi_1)} \right. \\ \left. + \frac{\kappa_\varepsilon (1 - 2\nu)}{E} \Delta P_{ext} - \frac{1}{\pi E} \frac{2\kappa_\varepsilon (1 - \nu)}{r_{0_{ext}}^2 - r_{0_{int}}^2} \delta F \right] \end{array} \right.$$

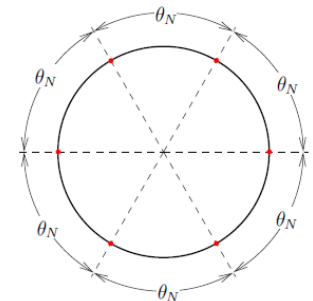

N sensors evenly arranged in ring position around the pipe

1 sensor = 1 pair of FBGs

$$|\varphi_1| \neq |\varphi_2| \pmod{\pi}$$



Additional effects mitigation & application to other measurement techniques

► The subtraction compensation process leads to a purely mechanical information

- **Temperature influence** on pressure measurement is **intrinsically cancelled**
 - Transducers sensitivity to temperature must be equal
- **Any additional effect**, different from purely mechanical, should also be **optimally mitigated**
 - e.g.: **nuclear radiations** influence on FBGs (responsible for Bragg wavelength shifts)
- The temperature ΔT information should therefore be considered as a global influence parameter
 - Including temperature, but also *any* additional non-mechanical influence on the transducers


► Application to other direction-sensitive surface strain or length measurement techniques

- The longitudinal mechanical strain variation $\Delta \varepsilon$ is nothing else but a relative length variation

$$\Delta \varepsilon = \ln \left(1 + \frac{\Delta L}{L} \right) \underset{0}{\sim} \frac{\Delta L}{L} \quad (\text{true longitudinal strain variation definition})$$

- Every measurement technique capable to measure length variations ΔL on pipe surface should also be able to perform non-intrusive pressure measurement
- Examples of candidate measurement techniques:

- **Ultrasonics** with PZT transducers
- **Non-contact** cross-correlation technique with video cameras for **remote pressure monitoring** (if sensitivity OK with regards to strain ranges)

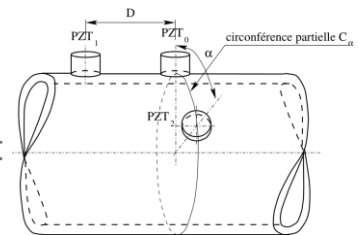

example of PZT transducers configuration distributed on pipe surface & dedicated to non-intrusive temperature self-compensated pressure measurement



FROM RESEARCH TO INDUSTRY

Experimental validations – From simple to more severe conditions

15:20-15:50, the 4th of March, 2022 – NURETH19 Workshop – Fiber-optic sensors for thermal hydraulic measurements







I – Mechanically isolated pipe section

► Pipe section filled with pressurized water

- No external force applied on the pipe – Room temperature
- Inflating pressure up to 300 bar
- Pipe length greater than 5 times its diameter
 - FBG transducers in the middle of the pipe section to be free from side effects

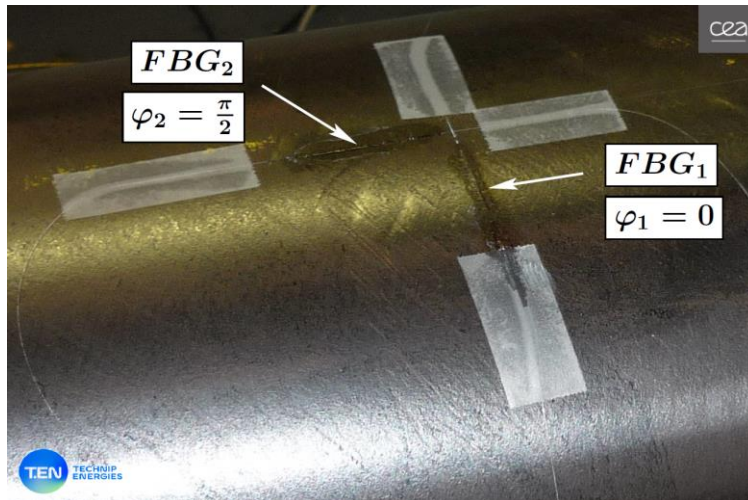

one non-intrusive FBG-based pressure sensor made of two FBG transducers in **hoop** and **longitudinal** configurations (best sensitivity configuration, also insensitive to torsion)

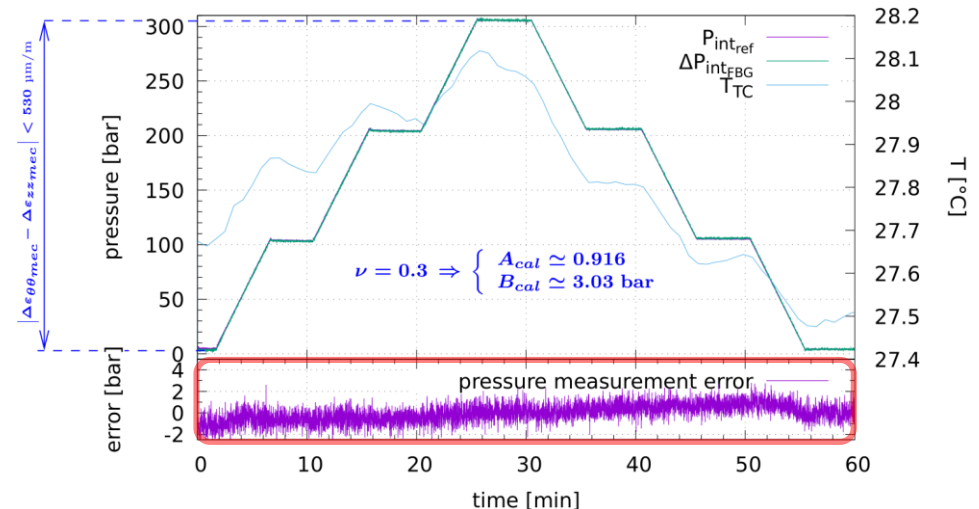

non-intrusive pressure **measurement error better than 0.54%**
Full Scale at 2σ after calibration – **5 Hz** measurement rate
 A_{cal} : calibration scale factor (*i.e.*: the gauge factor)
 B_{cal} : calibration pressure offset


measurement performed without delay (in real-time)




II – Air pressure loop

► Air pressure loop including several bends

- FBG transducers in the middle of a 5 m long pipe section – **Complex pipe layout with many bends**
- **Air flow rate steps up to 300 m³/h** – Room temperature

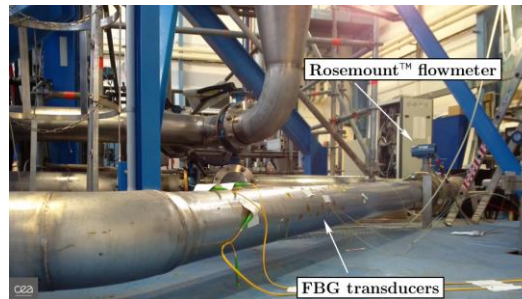



complex pipe layout including several **bends** and **attachments**

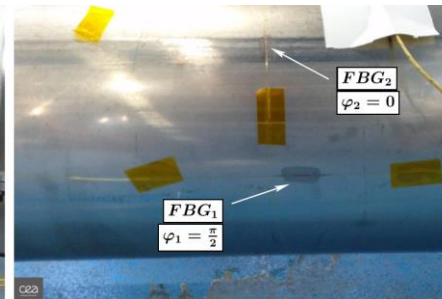

one non-intrusive pressure sensor made of two FBG transducers in **hoop** and **longitudinal** configurations (best sensitivity configuration, also insensitive to torsion)

thermocouples on pipe surface for reference temperature

Rosemount™ air flow rate Q : $Q_{[m^3/h]} = 3600 \times (0.02661 V_{[V]} - 0.02778)$

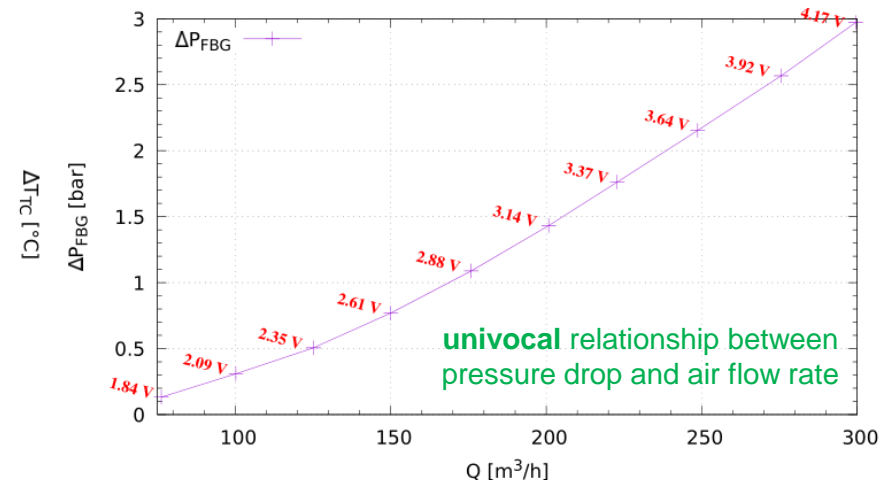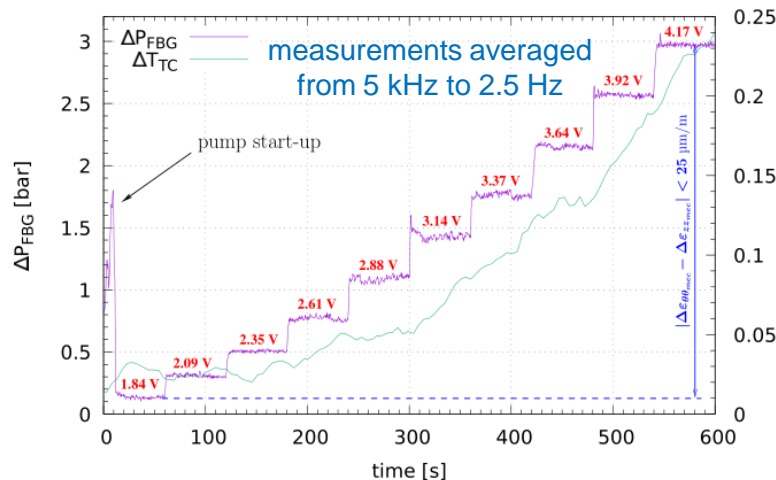



III – Water pressure loop (NPP primary coolant circuit)



► BEARN 2 water pressure loop (up to 320°C – 150 bar – 14 m³/h)

- FBG transducers installed on **Ø 2" NPS Sch. 80** and **Ø 4" NPS Sch. 160** pipe sections
- Non-intrusive sensors made of pairs of FBG transducers in **hoop** & **longitudinal** configurations
 - Rings configurations to mitigate bending effects

complex pipe layout
including several
bends and
attachments

inline **heaters** and
hydraulic pumps

valves to isolate pipe
sections from fluid flow

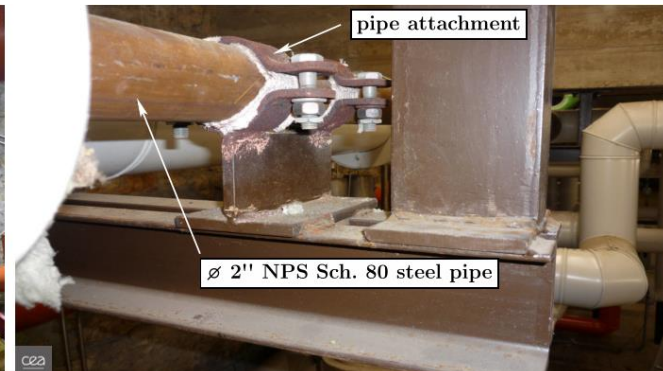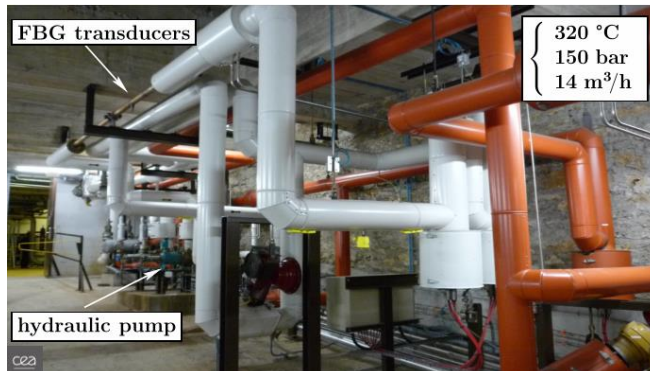

Ø 2" NPS Sch. 80

typical pipe attachment

Ø 4" NPS Sch. 160

► Typical orders of magnitude (see also page 12)

Ø 4" NPS Sch. 160 vs. Ø 2" NPS Sch. 80 steel pipes		Ø 4"	Ø 2"
$\Delta P_{int} = 100$ bar	$\Rightarrow \Delta \varepsilon_{\theta\theta_{mec}} - \Delta \varepsilon_{zz_{mec}}$	93.4 $\mu\text{m/m}$	133 $\mu\text{m/m}$
1 pm measurement error	\Rightarrow pressure measurement error δP_{int}	0.89 bar	0.62 bar
1°C temperature compensation error	\Rightarrow pressure measurement error δP_{int}	26.6 bar	18.6 bar
1 bar pressure resolution	\Rightarrow temperature compensation better than	0.038°C	0.054°C
1 bar pressure error	\Rightarrow unexplained longitudinal force variation δF	600 N	190 N



III – Water pressure loop (Ø 4" NPS Sch. 160 section)

► Hot-air gun experiment to estimate the non-intrusive pressure measurement robustness

- Measurements performed on Ø 4" NPS Sch. 160 metallic pipe section
- Hot-air temperature *estimated* greater than 100°C to generate **asymmetrical temperature distribution** around the pipe (**hot spot**)
- Typically 5 cm distance between FBG transducers in hoop & longitudinal configurations
 - Temperature difference between FBG transducers *estimated* greater than 40°C

→ Pressure bias smaller than **5 bar**


→ **Without compensation**, the measurement error would have probably been greater than **1000 bar**

$$T_{(1|2)} = \frac{a_1 T_1 + a_2 T_2}{a_1 + a_2}$$

a thermal effusivity

$T_{(1|2)}$ FBG surface temperature

medium	thermal effusivity $J \cdot m^{-2} \cdot K^{-1} \cdot s^{-1/2}$
air	5.54
water	1590
stainless steel 310	6922

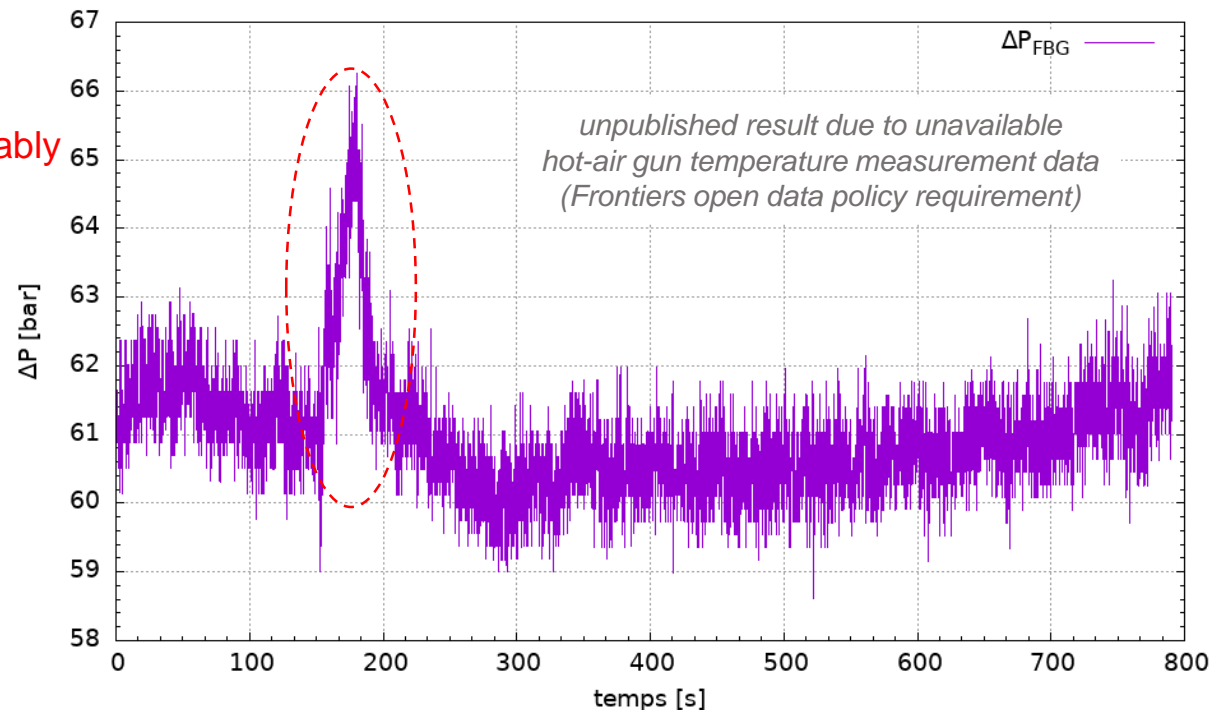



III – Water pressure loop (Ø 4" NPS Sch. 160 section)

► No fluid flow, no temperature change

single sensor configuration

bending mitigation configuration

reference intrusive pressure sensor

FBG pressure average error

1.36 bar (2σ)

bending mitigation with 3 FBG-based sensors ($\Rightarrow 3 \times 2 = 6$ FBGs) in ring configuration

\Rightarrow no significant improvement vs. single sensor measurement

► No fluid flow, but temperature changes due to heat conduction

- Closed instrumented section – Fluid flowing in the other part of the loop

single sensor configuration





bending mitigation configuration

$\Delta T_{max} \approx 19^\circ\text{C}$

FBG pressure average error

2.12 bar (2σ)


similar FBG surface temperature evolution than reference sensor

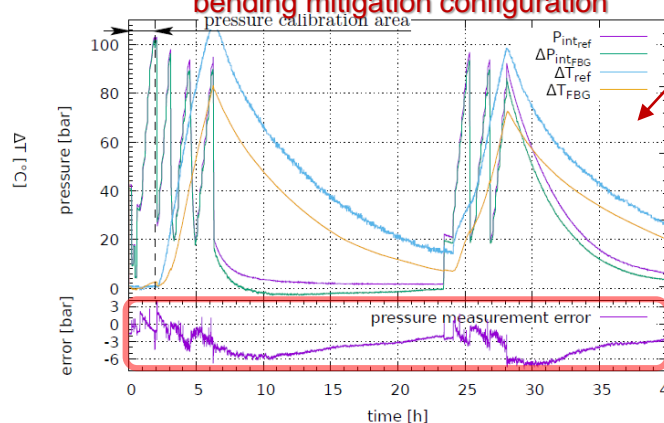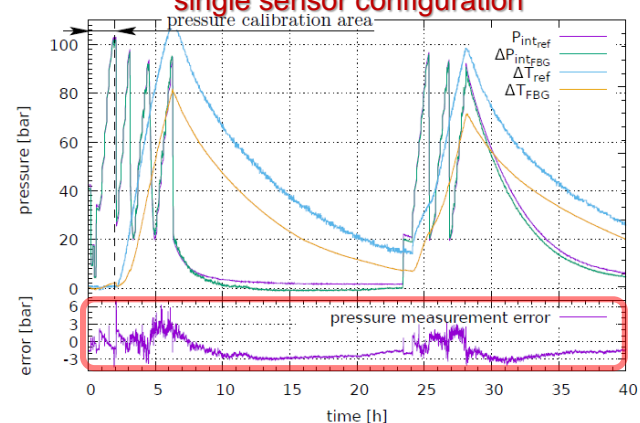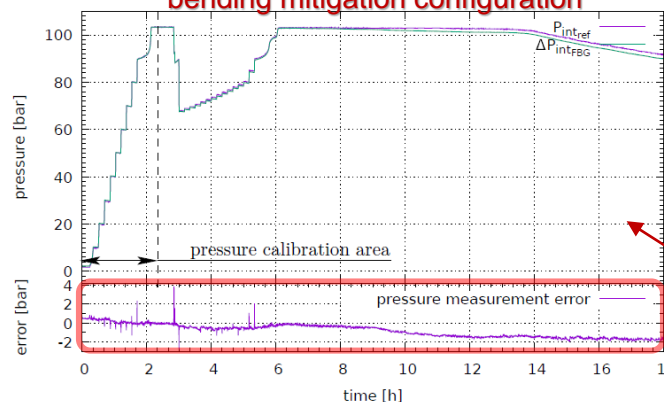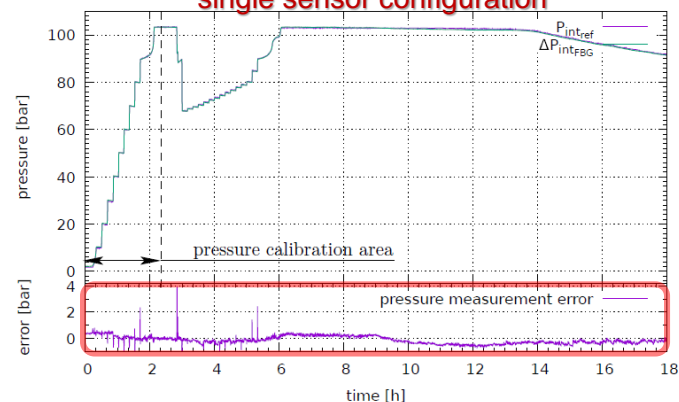



III – Water pressure loop (Ø 2" NPS Sch. 80 section)

► Fluid flow with massive fluid flow change (from 14 m³/h to zero) & temperature changes

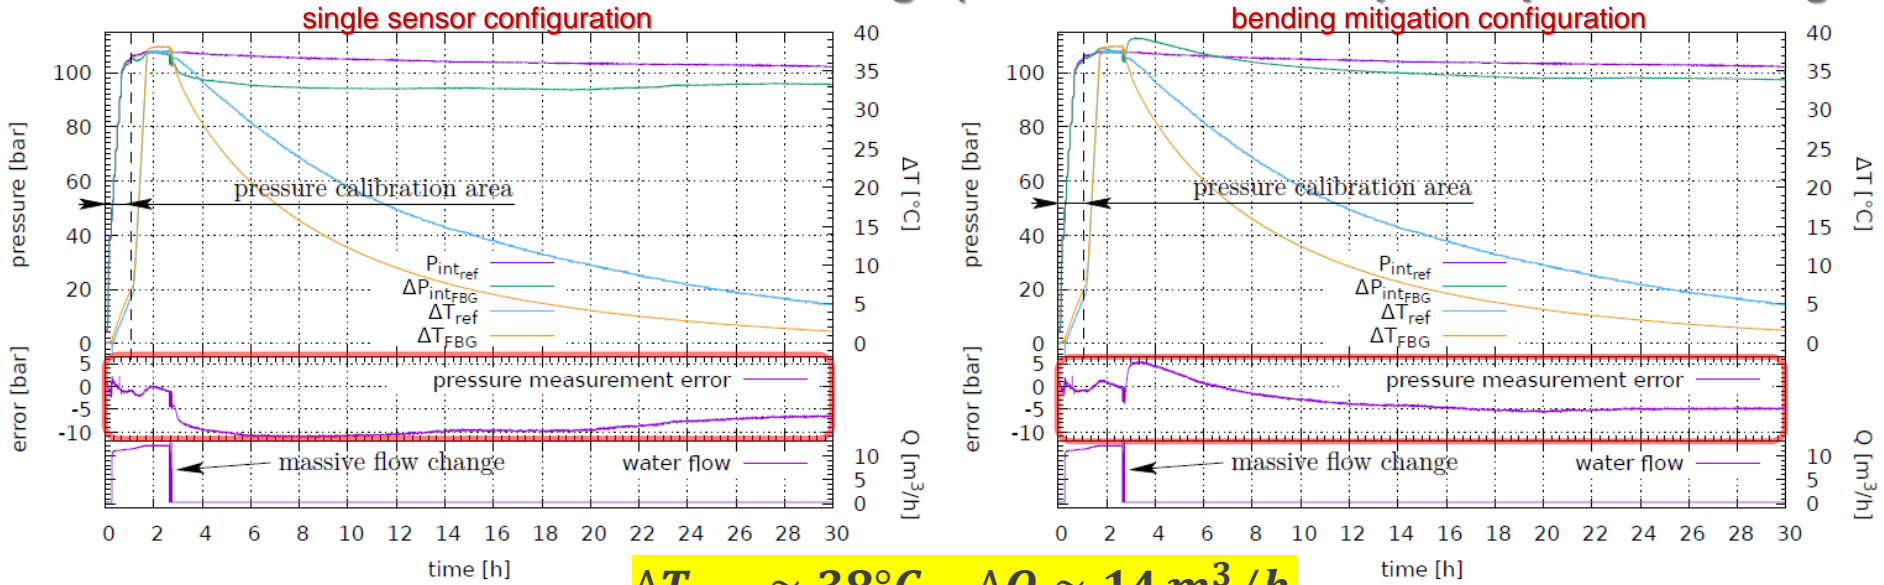


$$\Delta T_{max} \approx 38^{\circ}\text{C} - \Delta Q \approx 14 \text{ m}^3/\text{h}$$

- pressure calibration performed **during** important flow ΔQ and temperature ΔT changes
- FBG pressure average error **during calibration** close to **2 bar** (2σ)
- **similar** FBG surface temperature evolution than reference sensor

bending mitigation with 2 FBG-based sensors ($\Rightarrow 2 \times 2 = 4$ FBGs) in ring configuration

\Rightarrow **maximum pressure error roughly reduced by a factor of two vs. single sensor measurement, from -8.6 bar to -5 bar**

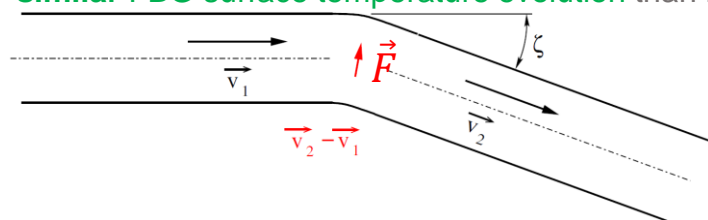

$$\vec{F} = \frac{d(m\vec{v})}{dt}$$

massive flow change, combined with fluid flow direction changes (bends), may generate significant bending forces \vec{F} on the pipe



FROM RESEARCH TO INDUSTRY

Conclusion

15:20-15:50, the 4th of March, 2022 – NURETH19 Workshop – Fiber-optic sensors for thermal hydraulic measurements



CEA - www.cea.fr

6 – 11 MARCH 2022, NURETH19, BRUSSELS, BELGIUM
19th International Topical Meeting on Nuclear Reactor Thermal Hydraulics




EUROPEAN NUCLEAR SOCIETY



Conclusion

- ▶ **Optimal temperature cross-sensitivity compensation is a key parameter for a reliable pressure measurement**
- ▶ **The closed pipe with circular cross-section provides an intrinsic mean to compensate for the transducers temperature cross-sensitivity with the same proof body**
 - The subtraction of two true relative raw measurements of direction-sensitive strain transducers is a purely mechanical information
 - Demonstrated by the linearized formal model for pipes with circular cross-section
 - Can probably be extended to other pipe cross-section shapes, but much more complicated to establish a dedicated formal model for demonstration...
 - In the elastic range, this information is proportional to the pipe internal pressure variation ΔP_{int}
 - The pipe surface temperature variation ΔT is an additional, but time delayed (due to heat diffusion in the pipe wall) information provided by the formal model, independently from the pressure information
- ▶ **Any additional non-mechanical effect can theoretically be intrinsically compensated**
 - e.g.: nuclear radiations on Bragg wavelengths for FBG transducers (but additional work necessary...)
- ▶ **Can be extended to any direction-sensitive surface strain or distance measurement**
 - Ultrasonics with PZT transducers
 - Non contact cross-correlation techniques (remote sensing)
- ▶ **Opens the way to new kinds of temperature self-compensated hydrostatic pressure sensors, based on a closed proof body with circular cross-section**
 - From tens to hundreds of bar in pressure ranges (depending of proof body mechanical properties and dimensions)

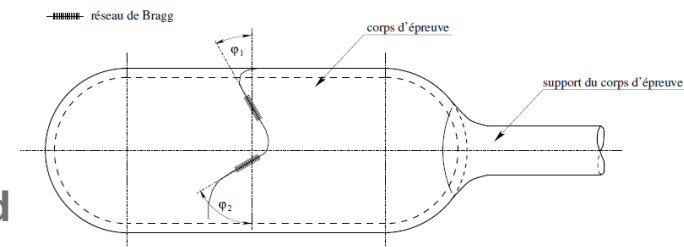

example of new kind of temperature self-compensated hydrostatic pressure sensor for *external pressure* P_{ext} monitoring



Acknowledgements

Additional information – Data availability





Acknowledgements

- ▶ **M. Daniel Mabilly** from **Technip Energies** for the kind permission to publish the data and the results from the pressure test held in **Marseille** in July 2019
- ▶ **M. Kévin Cruz** from **CEA DES IRESNE** for the pressure test held on **Mercure** facility in **Cadarache** in October 2019
- ▶ **M. Franck Ruffet** from **CEA DES DM2S** for his availability during the pressure tests held on **BEARN 2** facility in **Saclay** in 2020
- ▶ The **FSH public fund** which permitted to initiate the work on the formal model
- ▶ **M. Marc Baqué** and **TotalEnergies** which co-funded this research topic for a solution based on a different principle, but enabled us to benefit from the upgraded BEARN 2 pressure loop facility for this sensor
- ▶ **Prof. Patrice Mégret** from the **University of Mons** for the invitation to NURETH19 workshop





Additional information – Data availability

► This topic is published in *Frontiers in Sensors*, “Recent Advances in Optical Fiber Sensors”

- <https://www.frontiersin.org/research-topics/23029/recent-advances-in-optical-fiber-sensors>
- Original paper available at: <https://www.frontiersin.org/articles/10.3389/fsens.2022.835140>



► Publication in open access, with open data

- Open data will be made available in the CEA HAL open archive:

<https://hal-cea.archives-ouvertes.fr/cea-03541365>



Optimally temperature compensated FBG-based sensor dedicated to non-intrusive pipe internal pressure monitoring

Laurent Maurin¹*, Nicolas Roussel¹ and Guillaume Laffont¹

¹ Université Paris-Saclay, CEA, List, F-91120, Palaiseau, France

Correspondence*:

Laurent Maurin

¹Optic Fiber Sensors Laboratory, Metrology, Instrumentation and Information Department, List Institute, PC 72, CEA/Saclay, F-91191 Gif-sur-Yvette, France
laurent.maurin@cea.fr

ABSTRACT

Pipe internal pressure measurement is of utmost importance in the oil & gas industry to monitor the extraction process, and thus to prevent hydrate-plugs formation which may occur in specific temperature & pressure conditions. Traditional solutions usually rely on pressure sensors in direct contact with the fluid to monitor, therefore requiring one hole per sensor, but they also weaken the pipe structure, which may prematurely lead to significant leaks. Attempts to develop non-intrusive pressure sensors relying, for instance, on acoustic waves detection or even strain measurements (the pipe wall acting, in some way, like the membrane of a traditional intrusive sensor), are up to now not fully satisfying, mainly due to poor temperature cross-sensitivity compensation. Thus, 1°C temperature compensation error typically leads for Fiber Bragg Grating (FBG) transducers to pressure measurement biases greater than 26%@100 bar (e.g.: \varnothing 4" NPS Sch. 160 steel pipe). Consequently, if such non-intrusive, but biased, solutions could possibly have been considered to monitor, for instance, a Nuclear Power Plant (NPP) primary coolant circuit, it was with the risk of dramatic consequences since the fluid can reach temperatures up to 320°C. On the other hand, the solution detailed here truly achieves to cancel the temperature cross-sensitivity, and potentially any additional effect on pressure measurement, providing that each effect has the same influence on all transducers. It first relies on a better understanding of the pipe behavior under hydrostatic pressure, supported by a dedicated model developed on purpose, which demonstrates that the internal pressure & the surface temperature variations of a closed pipe can be recovered with at least two direction-sensitive transducers, the temperature dependence of the pressure measurement being simply removed by a straightforward compensation process. This paper explains the underlying principle, thanks to a formal model established with only few hypotheses, but extended to more complex field conditions. It ends with a lab-test validation involving FBG transducers attached to a pressure circuit submitted to temperature variations greater than several tens of °C, and concludes about the advantages & limitations of this novel approach for non-intrusive sensing, and its potential extensions to other measurement techniques.

Keywords: non-intrusive measurement, hydrostatic pressure, pipe, oil & gas, intrinsic temperature compensation, formal model, direction-sensitive transducer, Fiber Bragg Grating

1



Articles scientifiques du CEA
EN LIBRE ACCÈS

cea-03541365, version 1 Article dans une revue

Optimally temperature compensated FBG-based sensor dedicated to non-intrusive pipe internal pressure monitoring

Laurent Maurin¹, Nicolas Roussel¹, Guillaume Laffont¹ Details

¹ LCCO - Laboratoire Capteurs Fibres Optiques
DH2I - Département Métrologie Instrumentation & Information | DRT/LIST/DH2I

Abstract - Pipe internal pressure measurement is of utmost importance in the oil & gas industry to monitor the extraction process, and thus to prevent hydrate-plugs formation which may occur in specific temperature & pressure conditions. Traditional solutions usually rely on pressure sensors in direct contact with the fluid to monitor, therefore requiring one hole per sensor, but they also weaken the pipe structure, which may prematurely lead to significant leaks. Attempts to develop non-intrusive pressure sensors relying, for instance, on acoustic waves detection or even strain measurements (the pipe wall acting, in some way, like the membrane of a traditional intrusive sensor), are up to now not fully satisfying, mainly due to poor temperature cross-sensitivity compensation. Thus, 1°C temperature compensation error typically leads for Fiber Bragg Grating (FBG) transducers to pressure measurement biases greater than 26%@100 bar (e.g.: \varnothing 4" NPS Sch. 160 steel pipe). Consequently, if such non-intrusive, but biased, solutions could possibly have been considered to monitor, for instance, a Nuclear Power Plant (NPP) primary coolant circuit, it was with the risk of dramatic consequences since the fluid can reach temperatures up to 320°C. On the other hand, the solution detailed here truly achieves to cancel the temperature cross-sensitivity, and potentially any additional effect on pressure measurement, provided that each effect has the same influence on all transducers. It first relies on a better understanding of the pipe behavior under hydrostatic pressure, supported by a dedicated model developed on purpose, which demonstrates that the internal pressure & the surface temperature variations of a closed pipe can be recovered with at least two direction-sensitive transducers, the temperature dependence of the pressure measurement being simply removed by a straightforward compensation process. This paper explains the underlying principle, thanks to a formal model established with only few hypotheses, but extended to more complex field conditions. It ends with a lab-test validation involving FBG transducers attached to a pressure circuit submitted to temperature variations greater than several tens of °C, and concludes about the advantages & limitations of this novel approach for non-intrusive sensing, and its potential extensions to other measurement techniques.

Keywords: non-intrusive sensor | Hydrostatic Pressure | Pipe | Oil & gas | Surface temperature | intrinsic temperature compensation | bending mitigation | Formal model | Iterative algorithm | direction-sensitive transducer | FBG sensor | experimental validation | Pressure Loop | instrumentation | sensor | Optical Fiber Sensor | Fiber Bragg Grating | Distributed and Quasi-distributed sensing

Type de document Article dans une revue

Domaine Physique [physics] / Physique [physics] / Instrumentations et Détecteurs [physics.ins-det] | Sciences de l'ingénieur (physics) / Optique / photonique | Sciences de l'ingénieur (physics) / Traitement du signal et de l'image [eess.SP] | Sciences de l'ingénieur (physics) / Mécanique [physics.med-ph] / Matériaux et structures en mécanique [physics.class-ph]

IDENTIFIANTS
• HAL Id : cea-03541365, version 1
• DOI : 10.3389/fsens.2022.835140

COLLECTIONS
CEA | DRT | LIST | DH2I | OS-ENGINEERING | CEA-UPSAY | OS-COMPUTER-SCIENCE

CITATION
Laurent Maurin, Nicolas Roussel, Guillaume Laffont. Optimally temperature compensated FBG-based sensor dedicated to non-intrusive pipe internal pressure monitoring. *Frontiers in Sensors*. Frontiers Media, In press, 10.3389/fsens.2022.835140. (cea-03541365)

EXPORTER
BIBTeX | TEI | DC | ODC | EndNote

PARTAGER
f t e +

METRIQUES
Consultations de la notice
12

much more information about this sensor can be found in this article

this presentation will also be made available in the CEA HAL open archive

L. Maurin can be reached at laurent.maurin@cea.fr





Thank you for your attention

L. Maurin, N. Roussel & G. Laffont
Université Paris-Saclay, CEA, List, F-91120, Palaiseau, France

Credits: some of the pictures of this presentation are available under the [Creative Commons Attribution License \(CC BY\)](#)

