



HAL
open science

Using LVIC in current mode for energy spectrum reconstruction: experiments and validation

D Mazon, D Colette, E Soudet, P Malard, M Walsh, M Moreau

► To cite this version:

D Mazon, D Colette, E Soudet, P Malard, M Walsh, et al.. Using LVIC in current mode for energy spectrum reconstruction: experiments and validation. High-Temperature Plasma Diagnostics Conference 2022, May 2022, Rochester, United States. cea-03785814

HAL Id: cea-03785814

<https://cea.hal.science/cea-03785814>

Submitted on 23 Sep 2022


HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

INTRODUCTION

In tokamaks with Tungsten plasma facing components such as ITER, pollution of the plasma by heavy impurities is a major concern as it can lead to radiative breakdown. A diagnostic allowing reconstruction of the impurity distribution is thus of high interest. The radiation emitted by such impurities is mainly composed of soft X-rays (SXR) in the [0.1, 100] keV range. Due to the ITER radiative environment, in particular during high D-T power phase classic X-ray detectors such as semiconductor diodes might be too fragile and are thus not viable. Instead, advanced detectors (such as gas-filled detectors) are nowadays considered. The Low Voltage Ionization Chamber (LVIC) is one of the most promising candidate for X-ray measurement during the ITER nuclear phase [1]. A complete model of the detector recently developed at IRFM [2] now requires experimental validation.

LVIC SYNTHETIC DIAGNOSTIC

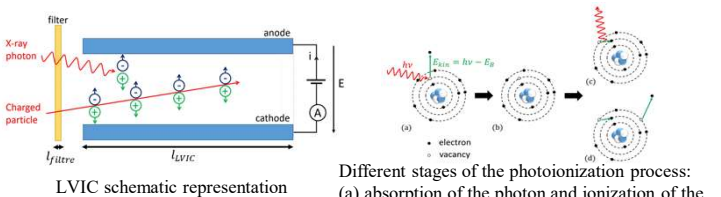

For a photon flux ϕ of energy $h\nu$:

- Coefficient of transmission through the filter:

$$T(h\nu) = \exp(-N_m * \sigma_{tot}(h\nu) * l_{filter})$$

- Coefficient of photoelectric absorption in the gas:

$$A(h\nu) = 1 - \exp(-N_g * \sigma_{ph}(h\nu) * l_{LVIC})$$

- X-ray fluorescence (if $h\nu > E_X$): Charge lost: $\Delta C_f = \frac{E_B}{W}$

For Argon, probability $P_f = 14\%$, $E_X = 3.2 \text{ keV}$, $E_B = 2.9 \text{ keV}$, $W = 26 \text{ eV}$ [3]

- Statistical fluctuations on the primary electron cloud N:

$$\frac{\sigma_N^2}{\langle N \rangle^2} = \frac{F}{\langle N \rangle}, \quad F = \text{Fano noise (0.23 for Argon)} [4]$$

A matrix computation is used

SOURCE CALIBRATION

Source calibration setup showing a Soft X-ray source (SRI SB-50-1k) with an aluminium filter (980 μm) and a Si Pin detector (XR-100CR) at a distance of 81 cm. Source spatial distribution is shown as a 2D heatmap of total number of counts. An acquired spectrum (over 15s) shows a peak at approximately 15 keV.

- Uniform spectrum on LVIC
- Good statistics in terms of counts
- W lines visible at 9.96keV and 11.42 keV

Acquired spectrum (over 15s)

EXPERIMENTAL RESULTS – MODEL VALIDATION

Experimental setup diagram shows a Soft X-ray source, aluminium filters (980 μm), and an LVIC detector at a distance of 81 cm. A photograph shows the physical setup with an amplifier and LVIC detector.

Al filter width (μm)	Measured Voltage (mV)	Simulated Voltage (mV)	Relative error (%)
980	7.36	7.71	4.5
0	191.22	203.29	5.9


SPECTRUM MODELING

Modeling of the spectrum using a simple mathematical function:

$$f(X) = \begin{cases} X_1 * \exp\left(-\frac{(h\nu - 9.961)^2}{0.03}\right) + X_2 * \exp\left(-\frac{(h\nu - 11.42)^2}{0.15}\right) + X_3 - X_4 * h\nu, & h\nu < 10 \text{ keV} \\ X_5, & 10 \text{ keV} < h\nu < h\nu_{lim} \\ 0, & h\nu_{lim} < h\nu < 30.11 \text{ keV} \\ 0, & h\nu > 30.11 \text{ keV} \end{cases}$$

SPECTRUM RECONSTRUCTION


Measuring currents with different filters allows the minimization of $r(X)$ to reconstruct the incoming spectrum: $\phi = f(X)$

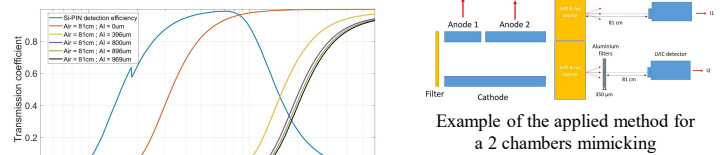

Transmission coefficient of Si-Pin and aluminium widths

$$\text{Chi-square minimisation } r(X) = \| I_{meas} - I(f(X)) \|_2^2$$

- Coherent spectrum reconstruction
- Bremsstrahlung nicely reproduced
- Discrete sets of current measurements associated to chi square minimisation are enough to get spectral information

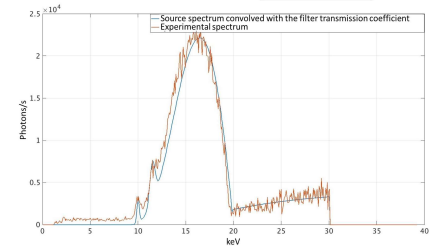

CONCLUSION

- LVIC synthetic modelling [2] has now been experimentally validated.
- The inversion method developed in [5] has been successfully applied to experimental measurements demonstrating the capability of a multi-chamber LVIC to reconstruct spectral information from a discrete set of measured current.
- Next step is to construct a multi-chamber LVIC and perform experimental testing on tokamaks.

References

[1] Y.V. Gott, M.M. Stepanenko, A low-voltage ionization chamber for the ITER, Instrum Exp Tech 52, 260-264 (2009), doi: 10.1134/S0020441209020250.
 [2] D. Colette, D. Mazon, R. Barnsley, A. Sirinelli, A. Jardin, M. O'Mullane, M. Walsh, Modeling a low voltage ionization chamber based tomography system on ITER, Rev. Sci. Instrum. 91, 073504 (2020); doi: 10.1063/1.5142909.
 [3] T. Watanabe, HW Schnopper, and FN Cirillo. "K X-ray fluorescence yield of argon", Physical Review 127.6 (1962), p. 2055
 [4] A. Hashiba, K. Masuda, T. Doke, T. Takahashi, and Y. Fujita. "Fano factor in gaseous argon measured by the proportional scintillation method", Nuclear Instruments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment 227.2 (1984), pp. 305–310. ISSN: 0168-9002. doi 10.1016/0168-9002(84)90138-4.
 [5] D. Colette, D. Mazon, R. Barnsley, M. O'Mullane, A. Jardin, A. Sirinelli, Conceptual study of energy resolved x-ray measurement and electron temperature reconstruction on ITER with low voltage ionization chambers, Rev. Sci. Instrum. 92, 083511 (2021), doi: 10.1063/1.5002846.